


# EC1/ES1 Electrostatic Speaker

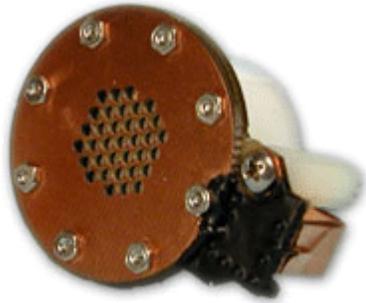

## Overview

TDT Electrostatic Speakers (Patent No. US 6,842,964 B1) are designed specifically for ultrasonic signal production. The electrostatic design offers a thin, flexible membrane with an extremely low moving mass. Unlike conventional speakers, these speakers distribute the driving signal homogeneously over the surface of the membrane. These factors produce a small, lightweight speaker with an excellent ultrasonic response and very low distortion. Available with or without a coupler, both models are easy to position and are particularly well suited for studies with small animals that have hearing in the ultrasonic range.

### **Part Numbers (Patent No. US 6,842,964 B1):**

ES1—Free Field Electrostatic Speaker

EC1—Electrostatic Speaker—Coupler Model

## Cable Connection

The ES1 and EC1 electrostatic speakers work exclusively with the ED1 Electrostatic Speaker Driver. Input is via a 4-pin, mini-DIN connector, which carries both bias and signal voltages from the speaker driver. Connection to the speaker driver is through a standard 6.1 m long cable. Other cable lengths can be special ordered, but will affect the speaker's frequency response. The speakers come fully enclosed to eliminate access to the high-voltage bias and driving signals. A 3.175 mm mounting hole at the base of the speaker accepts a standard 4-40 standoff. See "ED1 Electrostatic Speaker Driver" on page 16-15, for information about gain settings.

The orientation of the cable connection is indicated with dots on the cable connector and on the speaker. The cable should be connected so that the dot on the cable faces towards the speaker.

When connecting the cable, ensure that the four pin connectors are fully seated on the speaker and the speaker driver. When the cable is repeatedly moved during the experiment, periodically check that the connectors are fully seated.

## EC1 Coupled Electrostatic Speaker



The EC1 includes a small piece of Tygon® tubing coupled to the output. The tubing will transfer the signal best when it is kept straight. Note that the speaker performance is dependent on the coupling system used and the ear of the animal. Users should test the device under experimental conditions to ensure it meets their requirements. Technical Specifications measured under specific controlled conditions are provided for comparison purposes.

## Maximizing the Life of the Speakers

The TDT electrostatic speakers are designed to operate with input signals between 4 and 110 kHz. Playing signals below 4 kHz causes a large amount of harmonic distortion that degrades the operation of the speakers over time, causing a decreased power output across all frequencies.

### Broadband Signals

When using broadband signals, limit the amount of energy in the low frequency ranges whenever possible. For example, band limiting noise stimuli with a high pass filter at 4 kHz or above (the higher the better for the life of the speakers) and limiting complex harmonic signals, such as frequency sweeps, to frequencies above 4 kHz can increase the effective life of the speakers.

### Click Stimuli

ABR experiments in both human and mouse studies typically use a 100 microsecond click stimuli, which has most of its energy in the 2 kHz to 8 kHz range. Because click stimuli are short impulses that generate signals across a broad frequency range, band limiting the frequencies is not feasible. TDT recommends that users attenuate the click stimuli so as to minimize the potential effects on the speaker. Also note that the shorter the stimuli the flatter the frequency response and the greater the energy in the higher frequencies. Moreover, the shorter the duration of the click the less total energy it has (for a given voltage).

## Routine Care and Maintenance

Inspect speakers for visual damage or obstruction of the speaker holes prior to use. If there is damage to the copper shield around the components next to the connector or debris clogging the speaker holes, contact TDT for an RMA for repair.



**CAUTION!** NEVER attempt to clean the holes in the baseplate of the speaker. Doing so can puncture the speaker membrane.


When using the EC1, check the end of the Tygon® tubing for cerumen and other debris and clean as necessary.

## Technical Specifications


### ES1 Technical Specifications

Frequency Response	+/- 11 dB from 4 kHz to 110 kHz
Weight	22 Grams
Dimensions	3.8 cm outside diameter x 2.6 cm deep
Typical Output (10V peak input)	95 dB SPL at 10 cm, 5 kHz signal
THD	< 3%, 2 kHz - 110 kHz, 4 Vp input

### Free-field Frequency Response of Four Speakers at 10 cm

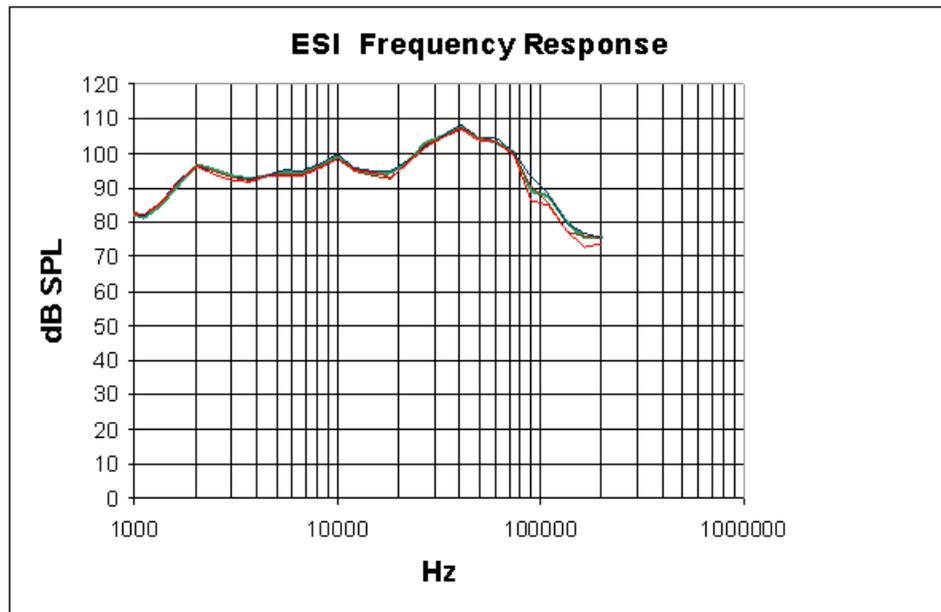

### Harmonic Distortion at 4 V Peak

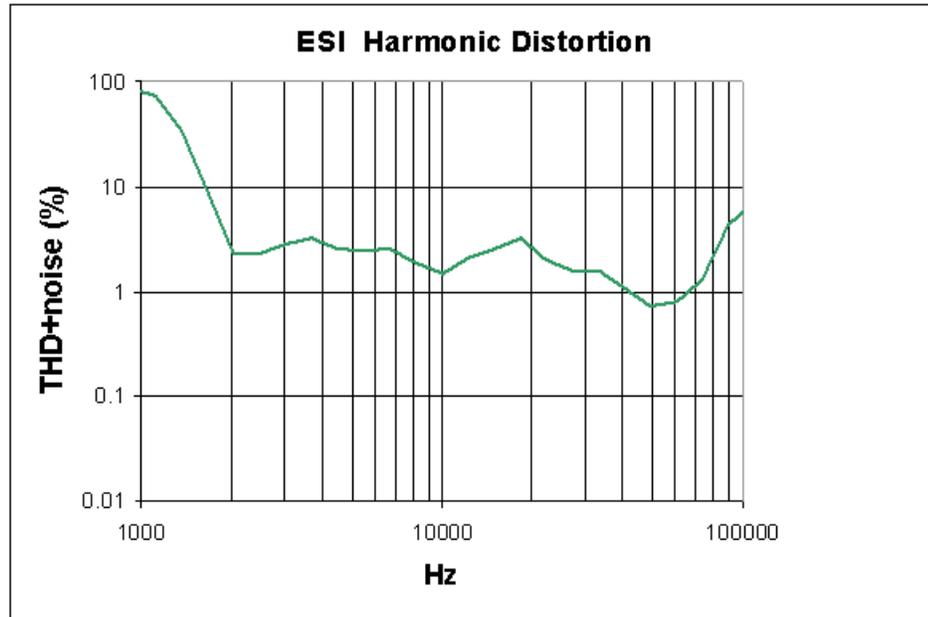

Noise as well as harmonic distortion is measured. Lower signal levels (e.g. above 75 kHz shown above) have higher THD+noise because of lower signal to noise ratios. When measured at higher signal levels, the THD above 75 kHz is actually <3% up to 110 kHz.

## EC1 Technical Specifications


<b>Frequency Response</b>	+/- 9 dB from 4 kHz to 110 kHz
<b>Weight</b>	22 Grams
<b>Dimensions</b>	3.8 cm outside diameter x 2.6 cm deep
<b>Typical Output</b>	90 dB SPL, 5kHz signal* <i>Every experimental setup is unique. It is important to calibrate the response of the speaker in each experimental setup.</i>
<b>THD</b>	<i>Every experimental setup is unique. It is important to calibrate the response of the speaker in each experimental setup.</i>

### Frequency Response in Plexiglas Coupler

\*Measurements were made in a 1 cm x 0.5 cm coupler with a 20 cm length of 2.4 mm i.e. tubing attached to the fitting of the EC1. 4 V peak input tones were tested and frequency response was measured with a calibrated pressure microphone.

The results of the calibration will vary depending on the type of ear to which the speaker is coupled and the length of the tube that is coupled to the ear. This curve

is provided as representative of the type of response that may be obtained in a closed field.

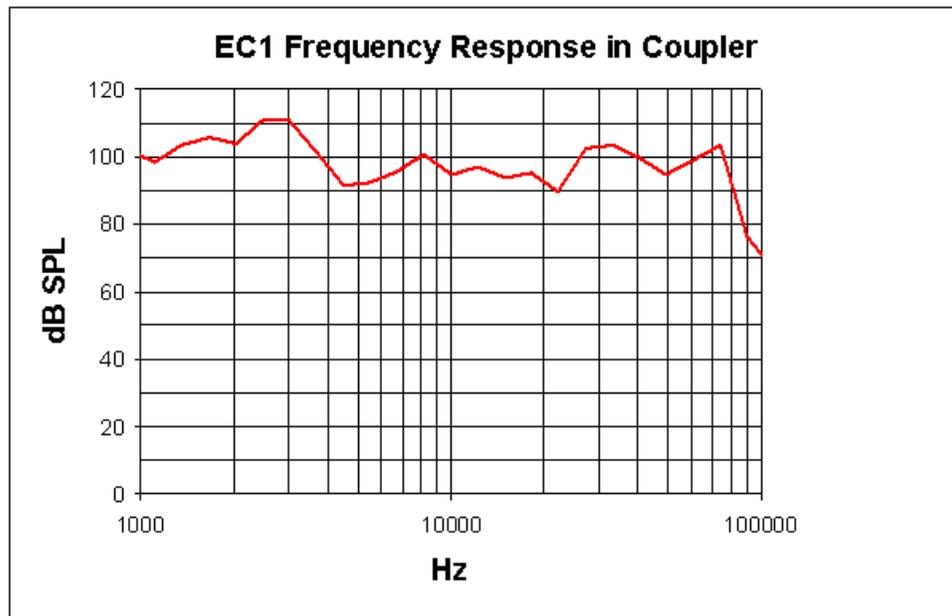

In this case, the low end of the response (< 5 kHz) is enhanced over the free-field response while the high end of the response (> 80 kHz) is attenuated.

**Every experimental setup is unique. It is important to calibrate the response of the speaker in each experimental setup.**

**Important!** Modifying the EC1 or ES1 can result in unexpected changes in the transfer function. All modifications to the EC1 or ES1 should be performed by TDT. If you need to be 30-60 dB lower than specifications, or if you have one of these devices, contact TDT for assistance.

